

Cold Chain Product Handling Note - Jynneos

ALABAMA
PUBLIC
HEALTH

Your cold chain shipment will arrive in a specially designed cold chain shipping container called a CREDO. Inside the CREDO, there will be a temperature monitoring device called a TempTale Bio monitor. Using the two correctly will ensure you have a viable product to prevent illness and save lives. Instructions for opening and returning the Credo and the TempTale are below, and they will also accompany the product shipment.

Please **“Reply to All”** in this message if you have any questions.


INSTRUCTIONS

1. Open the Credo cold chain shipping container.
2. View the TempTale and record the temperature you see as it may be important later.
3. Stop the TempTale monitor by pressing the STOP button for 1-3 seconds.
4. View the TempTale LCD to look for the alarm/bell shaped “Limits Exceeded” icon as shown below. If you do not see the limits exceeded icon, **your product is cleared for use**. Please move on to step 6 and return the TempTale and Credo to SNS.
5. If you DO see the limits exceeded icon (bell symbol), push and hold (approximately 3-5 seconds) the green START button to begin to take a close-up picture of EACH of the 5 readings displayed on the TempTale LCD screen and forward the pictures to SNS by replying to all in the email that provided your ETA. SNS staff will review the images and work to determine whether the product is cleared for use or if you need a replacement shipment.
6. **As soon as you can**, repackage the TempTale into the CREDO container, and send both back to the SNS using the return shipping label. If you did not receive a return shipping label, notify SNS immediately by “Reply to All” to the email that provided your ETA.

Stopping a TempTale 4 Monitor

Press and hold (1 to 3 seconds) the Stop button until the “Stop sign” ● icon appears in the upper right corner of the LCD display.

Displayed Information

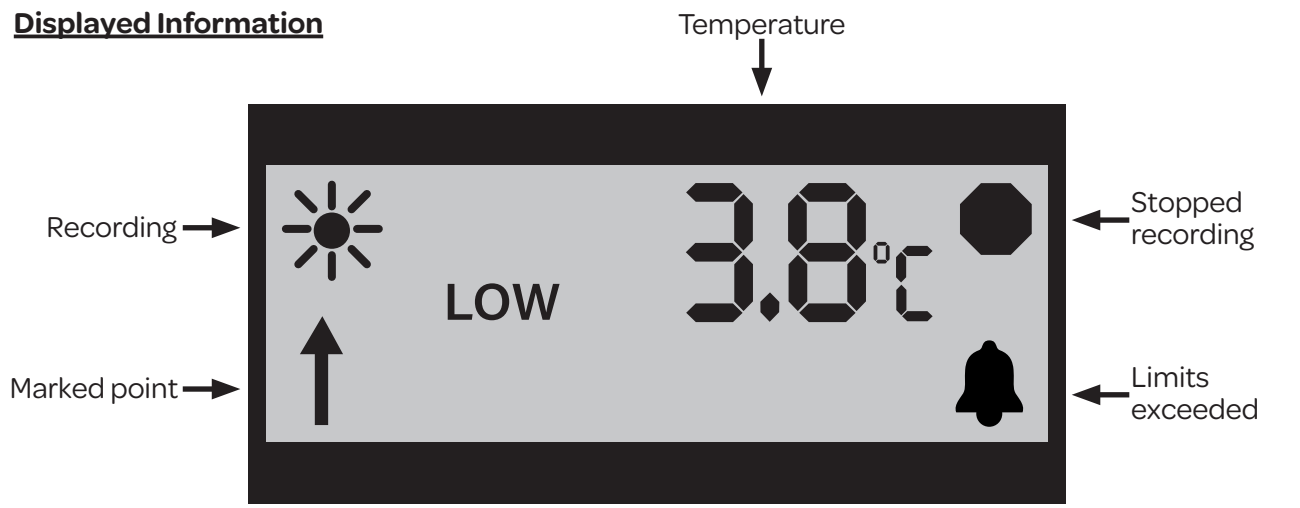

Note that the Jynneos Use During Mpox Response: Vaccine Accountability Form provided by CDC is no longer needed, so we no longer attach the form.